



MagPurix[®] Bacterial DNA Extraction Kit (ZP02006)

Instructions for Use (Handbook)



Version: 1.9



48



For *in vitro* diagnostic use



ZINEXTS LIFE SCIENCE CORP.
16F., No. 93, Sec. 1, Xintai 5th Rd.,
Xizhi Dist., New Taipei City 221416,
Taiwan (R.O.C.)



Obelis s.a.
Bd Général Wahis 53
1030 Brussels Belgium
Tel: +(32) 2 732-59-54
Fax: +(32) 2 732-60-03
mail@obelis.net

Read and follow these Instructions for Use prior to using this product. The latest revision of this document can be found at www.zinexts.com

Contents

Intended Use	3
Introduction	3
Kit Contents and Storage	4
Materials Required But Not Provided	5
Warnings and Precautions	5
Purification Principle	6
Before Starting	7
Preparation of sample materials	7
Procedure of MagPurix System	10
Purification Protocol - MagPurix® series	10
Purification Protocol - MagPurix® EVO	11
Troubleshooting	12
Related Products	13
References	13
Symbols	14
Limited Product Warranty	15
Revision History	15

Intended Use

The MagPurix® Bacterial DNA Extraction Kit provides a complete set of reagents and consumables for fully automated and simultaneous purification of bacterial nucleic acids from human biological specimens, inactivated pathogenic microorganism, bacterial pellet/colony from culture, clinical swab samples in liquid transport media, and environment material (water, soil, etc.) with MagPurix system.

The product is intended to be used by professional users, such as technicians and physicians who are trained in molecular biology techniques.

Introduction

Product Name	MagPurix® Bacterial DNA Extraction Kit
Catalogue Number	ZP02006
Product Overview	The MagPurix® Bacterial DNA Extraction Kit is designed to extract bacterial nucleic acids from human biological specimens, inactivated pathogenic microorganism, bacterial pellet/colony from culture, clinical swab samples in liquid transport media, and environment material (water, soil, etc.). The kit uses unique magnetic ZiBeads® technology and in combination with MagPurix® series automatic instruments, achieved superior product quality, consistent and high product yield and reproducible results. The final product is suitable for a wide range of diagnostic and research applications, such as sequencing, genotyping, qPCR, ddPCR and NGS assays.
Applicable Instrument Model	All MagPurix® Instrument
Display Protocol Name on The Instrument	2006 BACTERIAL DNA 2006 BACTERIAL RAPID (EVO only)
Applicable Instrument Firmware	Please check and download the latest firmware from www.zinexts.com
Processing Time	MagPurix® 12 series 55-70 minutes MagPurix® 24 series 65-80 minutes MagPurix® EVO 45-55 minutes (RAPID : 28-36 min)


Kit Contents and Storage

Shipping and Storage	The kit is shipped at room temperature. Upon receipt, store the kit at room temperature. All kit components are stable when stored properly until the expiration date shown on the kit box.	
Kit Content	The components supplied in the kit are listed below. Sufficient reagents are supplied to perform 48 purifications.	
	Contents	Amount
	1 Reagent Cartridge	48 pcs (6x8)
	2 Reaction Chamber	48 pcs (6x8)
	3 Tip Holder	48 pcs (6x8)
	4 Piercing Pin	50 pcs
	5 Filter tip	50 pcs
	6 Sample Tube (2 mL)	50 pcs
	7 Elution Tube (1.5 mL)	50 pcs
	BL2B Buffer (25 mL)	1 pc
	Barcode sticker (EVO only)	50 pcs

Reagent Cartridge Contents

Each Reagent Cartridge has 10 positions with 10 sealed well. Positions 1-10 contain wells filled reagents for this protocol.

Reagent	Well No.
Proteinase K Solution	1
Lysis Buffer 3	2
Binding Buffer 1	3
Magnetic Bead Solution	4
Washing Buffer 1B	5
Washing Buffer A	6
Washing Buffer B	7
Elution Buffer 1	8
Elution Buffer 2	9
Empty	10

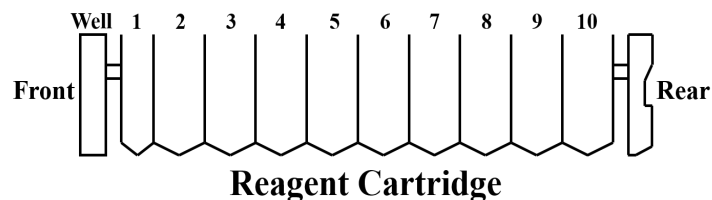

Materials Required But Not Provided

The following general laboratory equipment and consumables are required to perform the extraction. All laboratory equipment should be installed, calibrated, operated, and maintained according to the manufacturer's recommendations. The following tables display required and special equipment along with the list of consumables.

Item
MagPurix® series instruments
1.5 or 2.0 ml microcentrifuge tubes
Pipettes and filter tips
Phosphate-buffered saline (PBS, may be required for diluting samples)
Optional: Plastic consumables, DNase-free RNase A (to minimize RNA content)

Warnings and Precautions

For *in vitro* diagnostic use only. Read all the instructions carefully before using the kit. Use of this product should be limited to trained personnel in the techniques of DNA purification. Strict compliance with the user manual is required for optimal results. Attention should be paid to expiration dates printed on the box and labels of all components. Do not use a kit after its expiration date.


When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate safety data sheets (SDSs). These are available online in convenient and compact PDF format at <http://www.zinexts.com/download.php?lang=en&tb=1&cid=7> where you can find, view, and print the SDSs for each kit and kit component.

Please report any serious incident occurred in relation to the device to your local representative/agent or the manufacturer, and to the competent authority of your country/state.



CAUTION: DO NOT add bleach or acidic solutions directly to the sample preparation waste.

Purification Principle

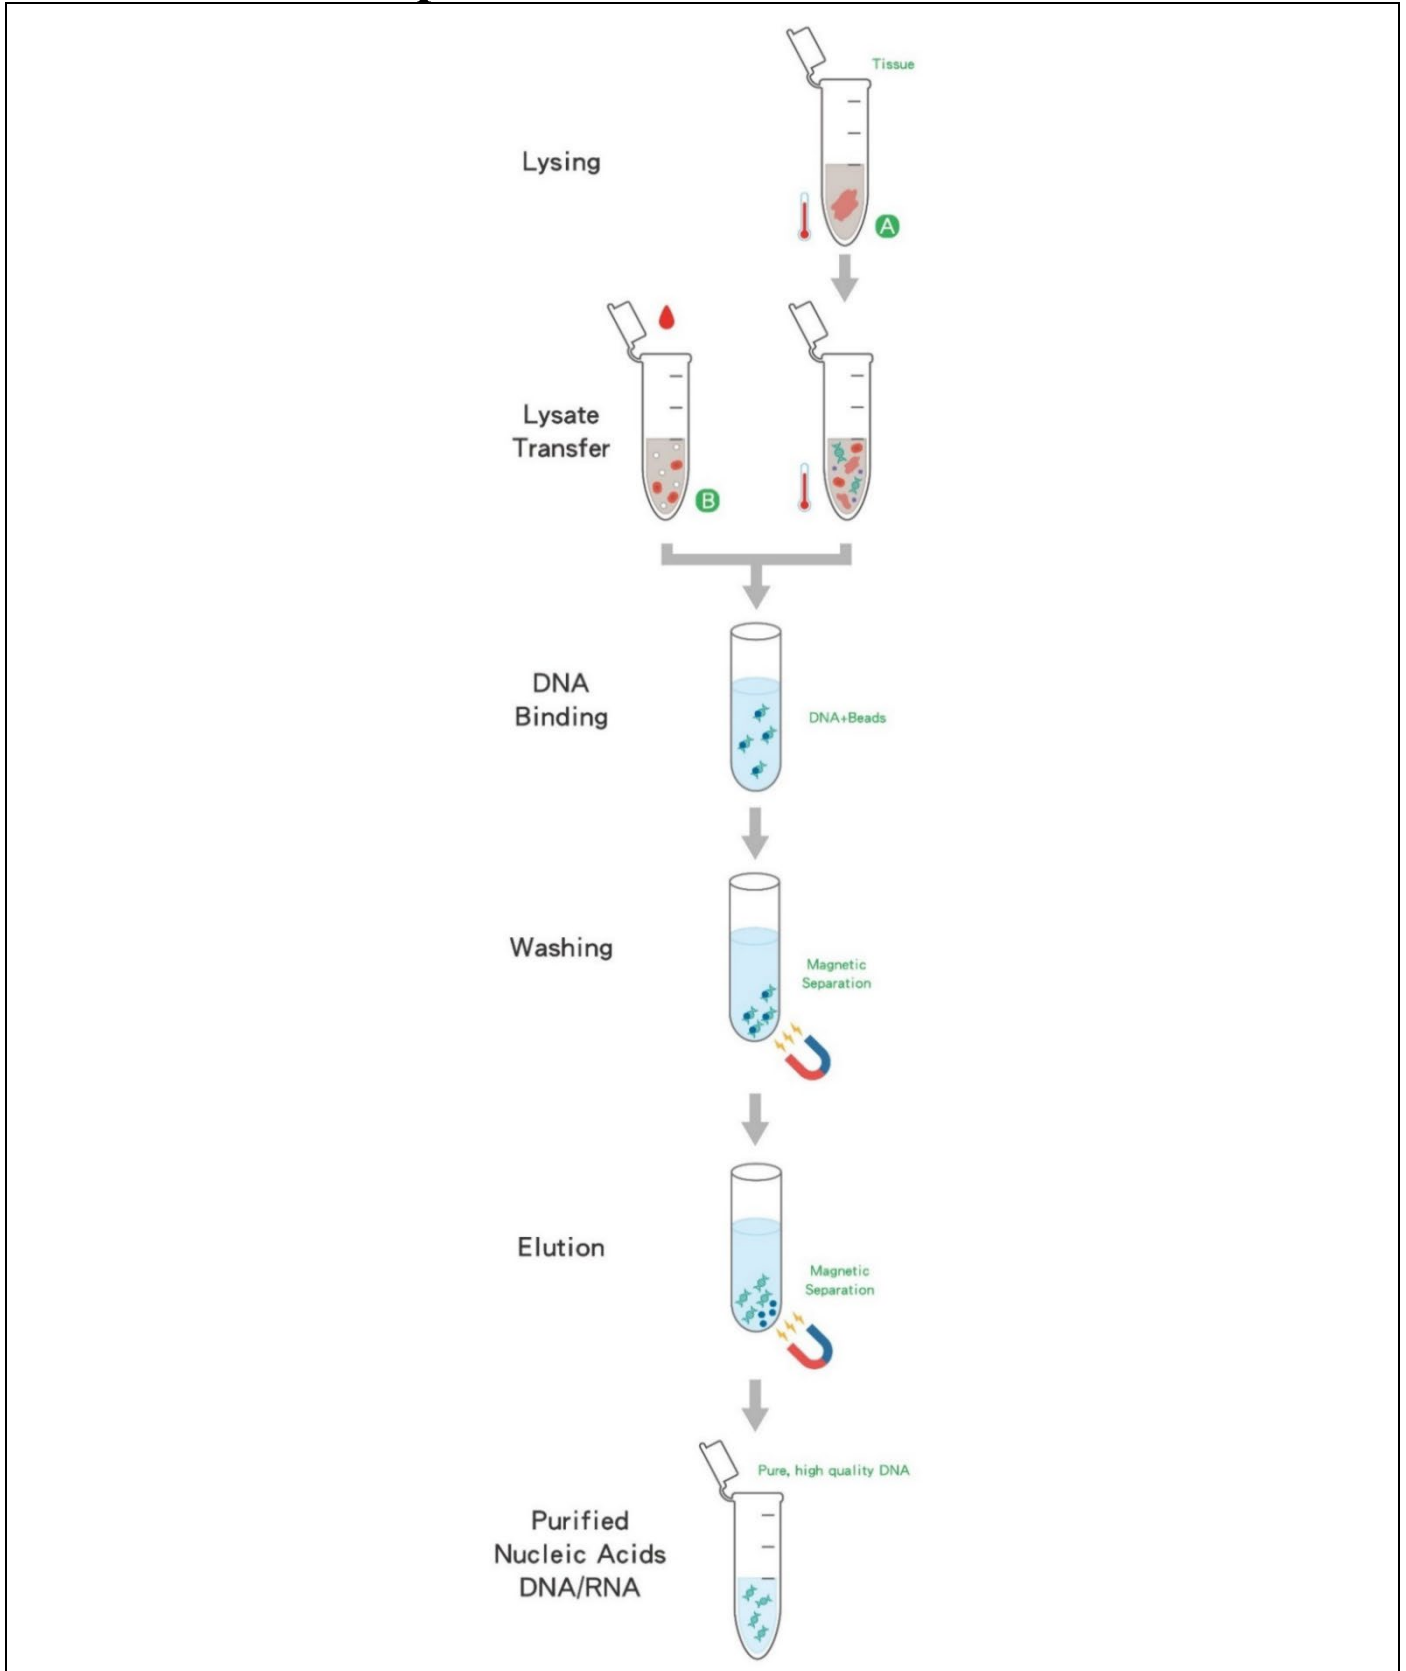

A Perform certain pretreatment process before extraction.

B Transfer sample to extraction directly.

Before Starting

Preparation of sample materials

The purification procedure is optimized for the use of 200-400 μ l inactivated pathogenic microorganism, bacterial pellet/colony from culture, clinical swab samples in liquid transport media or other cell-free body fluid samples.

Inactivation of pathogenic microorganism	<p>Method 1 - liquid samples (e.g. liquid transport media)</p> <ol style="list-style-type: none">Collect the samples in liquid transport media.Incubate for 10 minutes at 95°C.Centrifuge briefly to collect the complete sample volume at the bottom of the tube.Allow the samples to cool down or chill on ice.Transfer 200-400 μl to each Sample Tube. <p>Method 2 - Non-liquid samples (e.g. dry swab)</p> <ol style="list-style-type: none">Place the samples in 1 ml PBS containing a common fungicide.Incubate for 30 minutes at room temperature.Incubate for 10 minutes at 95°C.Pellet microorganism by centrifugation at 14,000 x g for 10 minutes.Discard supernatant, and then resuspend pellet in 220-440 μl BL2B Buffer.Transfer 200-400 μl suspension to each Sample Tube.
Viscous samples	<ol style="list-style-type: none">Collect viscous samples (e.g., BAL, sputum or other mucus specimen).Prepare a fresh DTT stock solution for liquefaction*. (e.g., 5X DTT stock is about 0.75%)Add DTT solution in the sample (final concentration: 0.15%).Incubate the sample (e.g., with shaking at 850 rpm for 30 minutes at 37°C) until it can be pipette easily.Pellet bacteria by centrifugation at 14,000 x g for 10 minutes.Discard supernatant, and then resuspend the pellet in 220 μl BL2B Buffer.Transfer 200 μl to each Sample Tube. <p>* The liquefaction could be done by using other solutions, such as NALC (N-Acetyl-L-Cysteine)-NaOH or other agents, which could digest mucous material.</p>
Solid animal tissue(s)	<ol style="list-style-type: none">Transfer the tissue to a 1.5 ml microcentrifuge tube. Cut tissue into small pieces or use a homogenizer to increase lysis efficiency and final DNA yield.Add 220-440 μl of BL2B Buffer to each sample and ensure that the tissue pieces are completely immersed in the buffer.Dispense 20 μl of proteinase K solution into each sample and vortex to mix.Incubate the tube in a shaking water bath or thermomixer at 55°C until the tissue is completely dissolved. If you do not have a shaker/mixer device, vortex or mix the sample every 5 min, until the tissue pieces dissolve. The lysis time depends on the type of tissue and is usually completed within 1-2 hours. However, overnight lysis is possible and does not affect the preparation. <p>* If the tissue cannot be completely dissolved, a larger amount of BL2B Buffer and/or proteinase K mixture is required.</p>

	<ul style="list-style-type: none"> e. Incubate the lysate at 70°C for 10 minutes to inactivate the activity of proteinase K. f. Spin down the treated lysate and transfer 200 µl into each Sample Tube.
Cell-free body fluid(s)	<ul style="list-style-type: none"> a. Pellet the bacteria by centrifugation at 14,000 x g for 15 minutes and discard the supernatant. b. Resuspend the pellet in 220 µl BL2B Buffer. c. Mix vigorously on a vortex mixer for 5-10 seconds. d. Transfer 200 µl supernatant into each Sample Tube.
Gram-positive bacterial species.	<ul style="list-style-type: none"> a. Follow the regular homogenization* procedures in the laboratory. b. For some sample types, DNA yield can be improved by performing this homogenization step prior to adding BL2B Buffer and Proteinase K. <p>* Especially for samples that contain particles (e.g., stool)</p>
Bacterial colony	<ul style="list-style-type: none"> a. Take 1-3 bacterial colony from culture plate with an inoculation loop and suspend in 220 µl BL2B Buffer by stirring vigorously. b. Transfer 200 µl suspension into each Sample Tube.
Bacterial suspension cultures	<ul style="list-style-type: none"> a. Add 1 ml bacterial culture into a 1.5 ml microcentrifuge tube and centrifuge at 5,000 x g for 5 minutes. b. Discard the supernatant. c. Add 220 µl BL2B Buffer to the pellet and vortex for 5-10 seconds. d. Transfer 200 µl suspension into each Sample Tube.
Swab samples	<p>Method 1 - Centrifuge</p> <ul style="list-style-type: none"> a. Collect swab samples (e.g., eye, nasal, pharyngeal, or other swabs) in liquid transport media or 1 ml PBS containing a common fungicide. b. Incubate for 30 minutes at room temperature. c. Pellet bacteria by centrifugation at 14,000 x g for 10 minutes. d. Discard supernatant, and then resuspend pellet in 220 BL2B Buffer. e. Transfer 200 µl suspension into each Sample Tube. <p>Method 2 - Centrifuge-free</p> <ul style="list-style-type: none"> f. Place the sample swab in 440 µl BL2B Buffer, incubate for 30 minutes at room temperature. g. Transfer 400 µl into each Sample Tube.
Large volume liquid samples	<ul style="list-style-type: none"> a. Centrifuge* sample at 10,000-16,000 x g for 5-10 minutes to concentrate bacterial cells into a pellet. b. Discard supernatant and resuspend the pellet in 220 µl BL2B Buffer.** c. Transfer 200 µl concentrated sample into each Sample Tube. <p>* Especially for samples that have low or unknown bacterial loads. (e.g., water collected from pool/river/stream/tower, soil, urine.)</p> <p>** If there were sand or other visible particle in the pellet, centrifuge again after BL2B Buffer treatment or filter out the dust.</p>

Use the paraffin-embedded tissue sections as samples, we recommend using the MagPurix® FFPE DNA Extraction Kit (ZP02009). If you use tissue as samples, we recommend using the MagPurix® Tissue DNA Extraction Kit (ZP02004).

Note:

The purification procedure is optimized for 200-400 µl of human biological specimens, inactivated pathogenic microorganism, cultured bacterial pellet/colony suspend in liquid buffer, clinical swab samples in liquid transport media, and environment material* (e.g., water, soil.).

*For large volume liquid samples with low or unknown bacterial content, e.g., water, soil, urine, or other, follow the recommended concentration procedure.

The BL2B Buffer is specialized for lysing bacterial cell wall** (supplied in the kit), please use it to resuspend the bacterial pellet or adjust sample volume before extraction.

**** For mycobacterium spp. (e.g., MTB), use BL3 Buffer for lysing bacterial cell wall {BL3 buffer is supplied in the MagPurix® TB DNA Extraction Kit (ZP02008)}.**

Using fresh sample (stored at 2-8°C for up to 6 hours) for extraction is recommended. Bacterial nucleic acid yield and quality will decrease with time or after multiple freeze–thaw cycles. For longer storage time, samples should be frozen at -20°C or lower and avoid freeze-thaw cycles. Thaw samples at room temperature (15-25°C) and process the sample immediately after equilibration to room temperature. **Do not** refreeze sample after thawing. If precipitation is visible in the sample, centrifuge at 6,800 x g for 3 minutes and transfer supernatant to a new tube without disturbing the precipitate, and immediately start the purification procedure.

The suggested starting material and elution volume range for each nucleic acid extraction.

Sample type	Starting material per sample	Elution Volume
Solid Animal Tissue(s)	200-400 µl / 1-30 mg	50-300 µl (EVO 50-200 µl)
Cell-free Body Fluids	200-400 µl	
Bacterial Pellet	200-400 µl NOTE: The sample amount is limited to up to 1×10 ⁹ cells/ml (OD600 = 3.0) bacteria.	
Bacterial Colony	1-3 bacterial colony	
Bacterial Suspension Cultures	200-400 µl	
Swab Samples	200-400 µl	
Environment Material	200-400 µl *large volume liquid sample pretreatment	
Pretreated Urine	200-400 µl *large volume liquid sample pretreatment	

Procedure of MagPurix System

Workflow of MagPurix operation

Place the cartridge and plastic consumables on the MagPurix instrument



Select the protocol and setup the condition



Follow onscreen message for worktable setup



Start the protocol



Collect elution product *



UV decontamination

* Output the bench record (option)


Note: Perform all steps at room temperature (20-25°C) unless otherwise notified.


Purification Protocol - MagPurix[®] series

1	Turn on the Instrument	a. Turn on the power switch and wait for the screen to turn on.
2	Load new Consumable(s) and Cartridge(s)	a. Open the door and remove the Sample Rack from the instrument. b. Load 1 Reagent Cartridge, and all plastic disposables (2 Reaction Chamber, 3 Tip Holder, 4 Piercing Pins, 5 Filtered Tips and other components presented in the kit intended to use). c. Place 6 Sample Tubes and 7 Elution Tubes into the Sample Rack.
3	Load the Samples	a. Transfer appropriate volume of sample into each Sample Tube on the Sample Rack. b. Put the Sample Rack back into the instrument and close the door.
4	Program Set up	a. Scan the protocol barcodes to select the purification protocol, sample volume and elution volume.
5	Start Extraction	a. Follow the instructions displayed on the screen to double-check the operating steps being completed before program running. b. Press " ENTER " to start the experiment. Instrument will run the protocol program automatically until the whole process is completed. c. At the end of the run (approximately 12 series 55-75 minutes , 24 series 65-80 minutes), instrument alarms briefly.
6	Collect the Elution tubes	a. Open the instrument door. b. Collect the elution tubes containing the purified nucleic acids. c. The purified nucleic acids are ready for immediate use. Store the purified nucleic acids at 4°C (short-term, less than 10 days) or aliquot and store at -70°C (long-term) before performing downstream analysis.

-
- d. Discard the used cartridges and all plastic consumables into biohazard waste. ***Do not reuse the cartridges.**
 - e. If you are not using the instrument immediately, place the Sample Rack back to the workplace, close the instrument door and press “Start” button for 2 seconds to enter sleep mode. Moreover, if the instrument will not be used in a long time, please turn off the power switch.
-

Purification Protocol - MagPurix[®] EVO

1	Turn on the Instrument	<ul style="list-style-type: none"> a. Turn on the power switch and wait for the screen to turn on. a. Login the instrument and enter the Home Page.
2	Load new Consumable(s) and Cartridge(s)	<ul style="list-style-type: none"> a. Open the door and remove the Sample Rack from the instrument. b. Open the Tip-Holder Lid. c. Load 1 Reagent Cartridge and all plastic disposables (2 Reaction Chamber, 3 Tip Holder, 4 Piercing Pins, 5 Filtered Tips and other components presented in the kit intended to use). d. Close the Tip-Holder Lid. e. Paste the barcode stickers on Elution Tubes. a. Place 6 Sample Tubes and 7 Elution Tubes into the Sample Rack.
3	Load the Samples	<ul style="list-style-type: none"> a. Transfer appropriate volume of sample into each Sample Tube on the Sample Rack. a. Put the Sample Rack back into the instrument and close the door.
4	Program Set up	<ul style="list-style-type: none"> a. Select the appropriate protocol program on the instrument. Press NEXT. b. Select the appropriate Sample Volume and Elution Volume and press NEXT. c. Press the number button to select the right Sample Numbers. d. Scan/Edit each primary Sample ID directly. After finished, press NEXT. e. Scan/Edit each Elution Tube ID directly. After finished, press NEXT. f. Scan Reagent Cartridge Barcode. Press NEXT. *If the cartridge is expired, the next step cannot be performed. a. Follow the instructions on the screen to double-check the operating steps being completed before running the program. Press NEXT.
5	Start Extraction	<ul style="list-style-type: none"> a. Check “PROGRAM CONFIRMATION” on the screen. b. Press “START” to start the experiment. Instrument will run the protocol program automatically until the whole process is completed. c. At the end of the run (approximately 45-55 minutes) (RAPID: 28-36 minutes), instrument alarms briefly and the screen indicates “PROGRAM FINISH”. d. If you want to perform the same protocol, press “RERUN” to perform the same experiment. If you do not need to re-run the experiment, press the function button “ HOME” to exist the experiment mode.
6	Collect the Elution tubes	<ul style="list-style-type: none"> a. Open the instrument door. b. Collect the elution tubes containing the purified nucleic acids.

- c. The purified nucleic acids are ready for immediate use. Store the purified nucleic acids at 4°C (short-term, less than 10 days) or aliquot and store at -70°C (long-term) before performing downstream analysis.
- d. Discard the used cartridges and all plastic consumables into biohazard waste. ***Do not reuse the cartridges.**
- e. If you are not using the instrument immediately, please put the Sample Rack back into the instrument, close the instrument door, and press the  **POWER** function button to enter sleep mode. If the instrument will not be used in a long time, please turn off the power switch.

Troubleshooting

***This table is helpful for solving common problem. If you need other technical support, please contact Zinexts team (<http://www.zinexts.com/index.php?lang=en>) or your distributor.**

Problem	Possible Cause	Comments and suggestions
Poor DNA quality or yield	Deterioration or contamination of reagents.	Please ensure that the reagents of kit are still in the effective use period before use. Discard any kit reagent that shows discoloration or evidence of microbial contamination.
	Kit stored under non-optimal conditions	Store kit at 15-25°C at all times after arrival. If either Reagent or Buffer precipitates upon shipping in cold weather or during long-term storage, dissolve precipitates by gently warming and stirring the solution. Please do not freeze the Reagent Cartridges.
	Insufficient sample input	DNA yield depends on the sample type and the number of nucleated cells in the sample. Please proportionally adjust the total input amount of sample to increase the DNA yield.
	Too much of elution buffer was used	The elution volume can be reduced proportionally.
	The eluent of final product(s) is not enough.	Please collect issue information and provide it to your Support Representative /Technical Support as soon as possible.
Clogged issue	Too much sample material was used.	Decrease the input amount of sample material or dilute your sample.
No results in downstream analysis	No signal/The PCR was inhibited.	Using appropriate controls for analysis. Check the positive control, negative control, water (NTC) and internal control to clarify the possible causes.

Instrument malfunction/abnormal sound	Abnormal consumables: 1. Deformed Filtered Tips 2. Deformed Reaction Chamber 3. Deformed Tip Holder	Please replace the batch with normal consumables.
	Abnormal action of instrument: 1. Inaccurate correction value 2. Spare parts or components damaged	Please collect issue information (videos and pictures) and provide it to your Support Representative/Technical Support as soon as possible to calibrate or replace any other damaged or worn parts.

Related Products












Product Name	Cat. no.
MagPurix® Blood DNA Extraction Kit 200	ZP02001
MagPurix® Blood DNA Extraction Kit 1200	ZP02002
MagPurix® Viral NA Extraction Kit	ZP02003
MagPurix® Tissue DNA Extraction Kit	ZP02004
MagPurix® Cultured Cell DNA Extraction Kit	ZP02005
MagPurix® Bacterial DNA Extraction Kit	ZP02006
MagPurix® HPV DNA Extraction Kit	ZP02007
MagPurix® TB DNA Extraction Kit	ZP02008
MagPurix® FFPE DNA Extraction Kit	ZP02009
MagPurix® Forensic DNA Extraction Kit	ZP02010
MagPurix® Viral Pathogen DNA Extraction Kit A	ZP02011
MagPurix® Viral Pathogen DNA Extraction Kit B	ZP02012
MagPurix® Viral RNA Extraction Kit	ZP02013
MagPurix® Plant DNA Extraction Kit	ZP02014
MagPurix® Total RNA Extraction Kit	ZP02015
MagPurix® Viral NA Extraction Kit LV	ZP02016
MagPurix® CFC DNA Extraction Kit	ZP02017
MagPurix® cfDNA Extraction Kit Plus	ZP02024
MagPurix® cfDNA Extraction Kit LV	ZP02025
MagPurix® Coronavirus RNA Extraction Kit	ZP02027

References

- Tan SC *et al.* J Biomed Biotechnol. (2009)

Symbols

The following symbols are used on labels and in Instructions for Use (IFU), in compliance with EN ISO 15223-1 standard.

Symbol	Explanation
	CE mark
	For In Vitro Diagnostic Use
	Catalogue number
	Lot/Batch number
	Sufficient for [n] samples
	Instructions for Use
	Expiry date
	Storage temperature (15°C - 25°C)
	Manufacturer
	European Authorized Representative
	Caution

Limited Product Warranty

Zinexts Life Science is committed to provide customers with high-quality products and services. Our goal is to ensure that every customer is 100% satisfied with our products and services. If you have any question or concerns, contact our Technical Support Representatives.

Zinexts Life Science guarantees the performance of all products according to the specifications stated in our product literature. The purchasers/users must determine the suitability of the product for their particular use. We reserve the right to change, alter, or modify any product to enhance its performance and design.

This warranty limits Zinexts Life Science Corporation's liability only to the cost of the product. No warranty is granted for products beyond their listed expiration date. No warranty is applicable unless all product components are stored and used in accordance with instructions.

Revision History

Version	Date	Description
1.9	11. Aug. 2022	List of IVD symbols added